




Title:


## Certificate of Analysis (CoA)

**Date:** 5/8/2026  
**Date Tested:** 5/5/2026  
**Customer:** Vertex Labs  
**Testing material:** Semax  
**Lot Number:** Sx0000038  
**BT Sample ID:** 005000039902713  
**Labeled Peptide Content/Potency:** 10 mg  
**Storage:** R.T.  
**Visual Description:** Small clear vial: white sample, white label, silver crimp, white plastic cap.  
**Labeled as:** Semax  
**Manufacturer:** Vertex Labs  
**Testing Purpose:** FTIR and HPLC analysis for the identification, purity, potency and composition of a peptide product. It does not provide information on particulate matter, microbial contamination or presence of endotoxins.



Test	Method	Specification	Result
General Appearance	USP <630>	white powder	white powder
Mass	USP <41>	As recorded	70.4 mg
FTIR Identification and Composition Analysis	USP <197A>	Sample spectrum should confirm the content of peptide via characteristic bands	FTIR sample spectrum confirms the presence of Semax with addition of excipient(s)/fillers.
HPLC Purity of Peptide Assay	USP <621>	Specifications: $\geq 98\%$	99.8 %
HPLC Potency Assay	USP <621>	Specifications: 90 – 110% of 10 mg	10.1 mg (101.2 %)
Peptide-to-Excipients Ratio	USP <1151>	Recommended ratios of (1:2) to (1:10) for (peptide: excipients)	10.1 : 60.3 mg (1:6)

The results of the CoA relate only to the item(s) tested and applied to the sample as received.

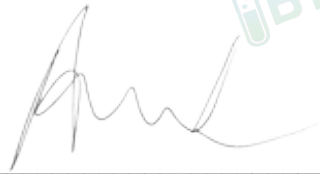

Andrea Castro, AS  
Scientist-II  
BTLabs




Verna Zheng, AS  
Scientist-II  
BTLabs




Title:

## Certificate of Analysis (CoA)

### FTIR ID and Composition Analysis: Semax Lot Sx0000038

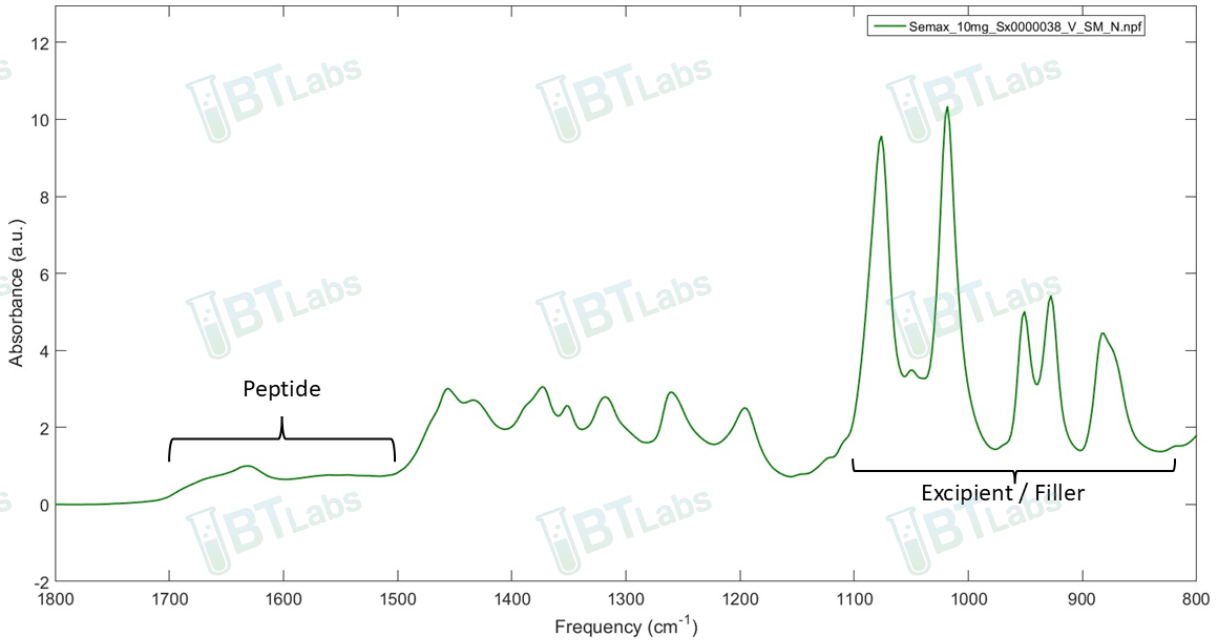

### HPLC Purity and Potency Assay @ 220 nm: Semax Lot Sx0000038

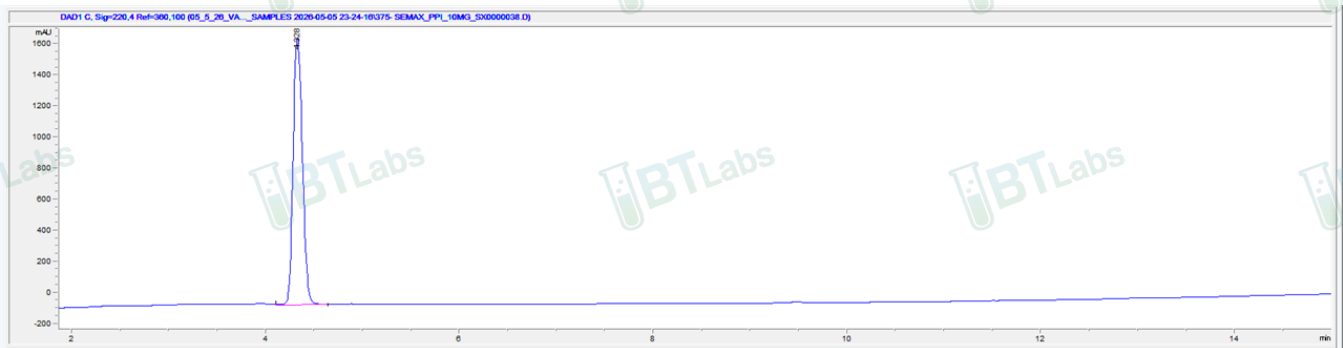

Semax Lot Sx0000038 @ 220 nm		
Peak #:	Retention Time (min)	Area (mAU*s)
1	4.328	180.7